


```
=====
Acq. Operator   : Liza                               Seq. Line :    2
Acq. Instrument : LC 1200                             Location  : Vial 2
Injection Date  : 7/14/2022 1:41:15 PM                Inj       :    1
                                                    Inj Volume: 10.0 µl

Sequence File   : C:\CHEM32\2\DATA\LIZA\ANALYSE DU FILTRAT KLASON1 -14-07-22 2022-07-14 13-
                  12-55\ANALYSE DU FILTRAT KLASON1 -14-07-22.S
Method          : C:\CHEM32\2\DATA\LIZA\ANALYSE DU FILTRAT KLASON1 -14-07-22 2022-07-14 13-
                  12-55\MONOSACCHARIDE JUILLET 2022_LIZA NEW.M (Sequence Method)
Last changed    : 7/8/2022 11:46:47 AM by Maxime2022
Method Info     : RID-2
=====
```

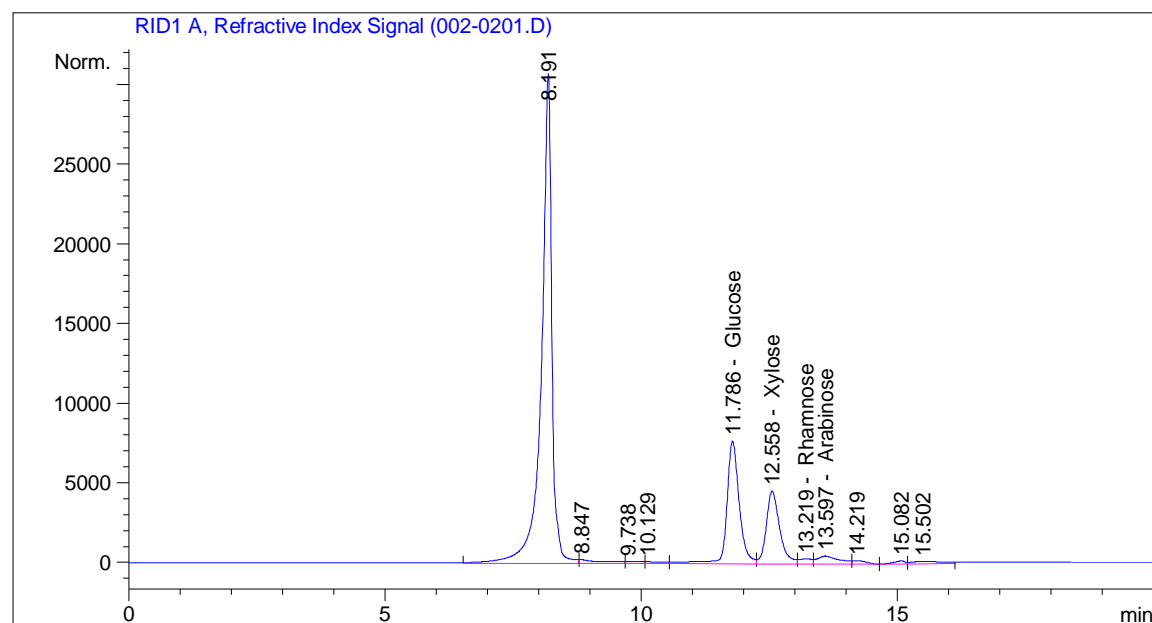

External Standard Report

```
Sorted By           :      Signal
Calib. Data Modified :      7/8/2022 11:11:10 AM
Multiplier:         :      1.0000
Dilution:           :      1.0000
Use Multiplier & Dilution Factor with ISTDs
```

Signal 1: RID1 A, Refractive Index Signal

RetTime [min]	Type	Area [nRIU*s]	Amt/Area	Amount	Grp	Name
11.786	VV	1.30907e5	5.52149e-6	7.22800e-1		Glucose
12.467		-	-	-		Mannose
12.523		-	-	-		Galactose
12.558	VV	8.29943e4	5.74771e-6	4.77027e-1		Xylose
12.696		-	-	-		Fructose
13.219	VV	5615.90039	1.51648e-5	8.51643e-2		Rhamnose
13.597	VV	1.50303e4	0.00000	0.00000		Arabinose

Totals : 1.28499

3 Warnings or Errors :

Warning : Calibration warnings (see calibration table listing)

Warning : Calibrated compound(s) not found

Warning : Negative results set to zero (cal. curve intercept), (Arabinose)

=====

*** End of Report ***